

User Guide

MILLIPLEX® Human Complement C5b-9 Singleplex Magnetic Bead Panel

96-Well Plate Assay

HC5B9-140K

Introduction.....	2	Immunoassay Procedure	16
Principle.....	3	Plate Washing.....	18
Storage Conditions Upon Receipt.....	4	Solid Plate.....	18
Reagents Supplied	5	Filter Plate	18
Human Complement C5b-9 Antibody- Immobilized Magnetic Beads.....	5	Equipment Settings.....	18
Materials Required	6	Quality Controls	19
Reagents.....	6	Assay Characteristics.....	20
Instrumentation/Materials	6	Cross-Reactivity	20
Safety Precautions	6	Assay Sensitivities	20
Symbol Definitions.....	7	Precision.....	20
Technical Guidelines	10	Accuracy.....	20
Sample Collection and Storage	12	Troubleshooting.....	21
Preparation of Serum Samples	12	Product Ordering	26
Preparation of Plasma Samples	12	Well Map	27
Preparation of Tissue Culture Supernatant	12	Notice	28
Preparation of Reagents for Immunoassay.....	13	Technical Assistance	28
Preparation of Antibody- Immobilized Beads	13	Standard Warranty	28
Preparation of Quality Controls	13	Contact Information	28
Preparation of Wash Buffer	13	Safety Data Sheets (SDS).....	28
Preparation of Standard Matrix	13		
Preparation of Human Complement C5b-9 Standard.....	14		

Introduction

The complement system consists of many plasma proteins that assist, or complement, the ability of phagocytic cells and antibodies to clear pathogens. Although it is part of the innate immune system, it can be recruited and activated by the adaptive immune system. The complement proteins and glycoproteins that are synthesized primarily by hepatocytes normally circulate as inactive pro-proteins. Once stimulated the result of the cascade is a massive amplification of response and activation of the membrane attack complex (C5b-9), which forms a transmembrane pore causing osmotic lysis of target cells. The complement pathway may also form soluble C5b-9, as well as intermediate isoforms, stabilized by regulatory proteins. These soluble complexes are unable to insert into the lipid membrane, and their role in complement pathways is an area of ongoing research.

The MILLIPLEX® portfolio offers the broadest selection of analytes across a wide range of disease states and species. Once the analytes of interest have been identified, you can rely on the quality that we build into each kit to produce results you can trust. In addition to the assay characteristics listed in the protocol, other performance criteria evaluated during the verification process include: cross-reactivity, dilution linearity, kit stability, and sample behavior (for example detectability and stability).

Each MILLIPLEX® panel and kit includes:

- Quality controls (QCs) provided to qualify assay performance
- Comparison of standard (calibrator) and QC lots to a reference lot to ensure lot-to-lot consistency
- Optimized serum matrix to mimic native analyte environment
- Detection antibody cocktails designed to yield consistent analyte profiles within panel

In addition, each panel and kit meet stringent manufacturing criteria to ensure batch-to-batch reproducibility. The MILLIPLEX® Human Complement C5b-9 Singleplex Magnetic Bead Panel thus enables you to focus on the therapeutic potential of complement factors. Coupled with the Luminex® xMAP® platform in a magnetic bead format, you receive the advantage of ideal speed and sensitivity, allowing quantitative multiplex detection of dozens of analytes simultaneously, which can dramatically improve productivity.

MILLIPLEX® Human Complement C5b-9 – Singleplex Magnetic Bead Panel is part of the most versatile system available for complement factor research. From our single to multiplex biomarker solutions, we partner with you to design, develop, analytically verify, and build the most comprehensive library available for protein detection and quantitation.

MILLIPLEX® kits offer you:

- A convenient “all-in-one” box format that gives you the assurance that you will have all the necessary reagents you need to run your assay.

MILLIPLEX® Human Complement C5b-9 – Singleplex Magnetic Bead Panel is a Singleplex kit to be used for the quantification of the following analyte in serum, plasma, or cell culture supernatant samples: C5b-9 (Membrane Attack Complex, Terminal Complement Complex).

For research use only. Not for use in diagnostic procedures.

For Research Use Only. Not for Use in Diagnostic Procedures.

Please read entire protocol before use.

It is important to use same assay incubation conditions throughout your study.

Principle

MILLIPLEX® kits are based on the Luminex® xMAP® technology — one of the fastest growing and most respected multiplex technologies offering applications throughout the life sciences and capable of performing a variety of bioassays including immunoassays on the surface of fluorescent-coded magnetic beads known as MagPlex® microspheres.

- Luminex® uses proprietary techniques to internally color-code microspheres with two fluorescent dyes. Through precise concentrations of these dyes, distinctly colored bead sets of 500 5.6 µm polystyrene microspheres or 80 6.45 µm magnetic microspheres can be created, each of which is coated with a specific capture antibody.
- After an analyte from a test sample is captured by the bead, a biotinylated detection antibody is introduced.
- The reaction mixture is then incubated with Streptavidin-PE conjugate, the reporter molecule, to complete the reaction on the surface of each microsphere.
- The following Luminex® instruments can be used to acquire and analyze data using two detection methods:
- The Luminex® analyzers Luminex® 200™, FLEXMAP 3D®, and xMAP® INTELLIFLEX are flow cytometry-based instruments that integrate key xMAP® detection components, such as lasers, optics, advanced fluidics and high-speed digital signal processors.
- The Luminex® analyzer, MAGPIX®, is a CCD-based instrument that integrates key xMAP® capture and detection components with the speed and efficiency of magnetic beads.
- Each individual microsphere is identified, and the result of its bioassay is quantified based on fluorescent reporter signals. We combine the streamlined data acquisition power of Luminex® xPONENT® acquisition software with sophisticated analysis capabilities of MILLIPLEX® Analyst 5.1, integrating data acquisition and analysis seamlessly with all Luminex® instruments.
- xMAP® INTELLIFLEX runs on INTELLIFLEX software for instrument control, run setup and generating high quality data with flexible output options. Data can be exported in xPONENT® style CSV files for compatibility with many existing analytical applications, or in the new, customizable INTELLIFLEX file format. The INTELLIFLEX file format is intended for flexibility and simplicity, allowing the user to freely select which data points to include and to reduce the time to analysis.

The capability of adding multiple conjugated beads to each sample results in the ability to obtain multiple results from each sample. Open-architecture xMAP[®] technology enables multiplexing of many types of bioassays reducing time, labor and costs over traditional methods.

Storage Conditions Upon Receipt

- Recommended storage for kit components is 2-8 °C.
- For long-term storage, freeze reconstituted standards and controls at ≤ -20 °C. Avoid multiple (> 2) freeze/thaw cycles.
- DO NOT FREEZE Antibody-Immobilized Beads, Detection Antibody, and Streptavidin-Phycoerythrin.

Reagents Supplied

Reagents	Volume	Quantity	Catalogue No.
Human Complement C5b-9 Standard	1 vial	Lyophilized	HC5B9-8140
Human Complement C5b-9 Quality Controls 1 and 2	1 vial each	Lyophilized	HC5B9-6140
Standard Matrix	1 vial	Lyophilized	MXHSM-C5B9
Bead Diluent	1 vial	3.5 mL	LBD
Set of one 96-Well Plate with 2 sealers	1 plate 2 sealers	-	-
Assay Buffer	1 bottle	30 mL	L-AB4
10X Wash Buffer	1 bottle	60 mL	L-WB
Human Complement C5b-9 Detection Antibodies	1 bottle	3.2 mL	HC5B9-1140
Streptavidin-Phycoerythrin	1 bottle	5.5 mL	L-SAPE5
Mixing Bottle	1 bottle	-	-

Included Human Complement C5b-9 Antibody-Immobilized Beads are listed on the next page.

Human Complement C5b-9 Antibody-Immobilized Magnetic Beads

Bead/Analyte Name	Luminex® Magnetic Bead Region	1 Analyte (20X concentration, 200 µL)	
		Available	Catalogue No.
Anti-human Complement C5b-9	56	✓	HC5B9-MAG

For research use only. Not for use in diagnostic procedures.

Materials Required (Not provided)

Reagents

MAGPIX® Drive Fluid PLUS (Catalogue No. 40-50030), xMAP® Sheath Fluid PLUS (Catalogue No. 40-50021), or xMAP® Sheath Concentrate PLUS (Catalogue No. 40-50023).

Instrumentation/Materials



- Adjustable Pipettes with Tips capable of delivering 25 µL to 1000 µL
- Multichannel Pipettes capable of delivering 5 µL to 50 µL, or 25 µL to 200 µL
- Reagent Reservoirs
- Polypropylene Microfuge Tubes
- Rubber Bands
- Aluminum Foil
- Absorbent Pads
- Laboratory Vortex Mixer
- Sonicator (Branson Ultrasonic Cleaner Model No. B200 or equivalent)
- Titer Plate Shaker (VWR® Microplate Shaker Catalogue No. 12620-926 or equivalent)
- Luminex® 200™, HTS, FLEXMAP 3D®, MAGPIX® with xPONENT® software or xMAP® INTELLIFLEX with INTELLIFLEX software by Luminex® Corporation.
- Automatic Plate Washer for magnetic beads (BioTek® 405 LS and 405 TS, Cat. Nos. 40-094, 40-095, 40-096, 40-097 or equivalent) or Handheld Magnetic Separation Block (Catalogue No. 40-285 or equivalent).



Note: If a plate washer or handheld magnetic separation block for magnetic beads is not available, one can use a microtiter filter plate (Catalogue No. MX-PLATE) to run the assay using a Vacuum Filtration Unit (Vacuum Manifold Catalogue No. MSVMHTS00 or equivalent with Vacuum Pump Catalogue No. WP6111560 or equivalent).




Safety Precautions

- All blood components and biological materials should be handled as potentially hazardous. Follow universal precautions as established by the Centers for Disease Control and Prevention and by the Occupational Safety and Health Administration when handling and disposing of infectious agents.
- Sodium azide or ProClin™ has been added to some reagents as a preservative. Although the concentrations are low, Sodium azide and ProClin™ may react with lead and copper plumbing to form highly explosive metal azides. Dispose of unused contents and waste in accordance with international, federal, state, and local regulations.

Symbol Definitions

Ingredient	Catalogue No.	Label	
Human Complement C5b-9 Standard	HC5B9-8140		<p>Danger. Causes serious eye damage. Harmful if inhaled. May cause damage to organs Respiratory Tract through prolonged or repeated exposure. Harmful to aquatic life with long lasting effects. Do not breathe dust. Use only outdoors or in a well-ventilated area. Avoid release to the environment. Wear eye protection/ face protection. IF INHALED: Remove person to fresh air and keep comfortable for breathing. Call a POISON CENTER/ doctor if you feel unwell. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. Get medical advice/ attention if you feel unwell. Dispose of contents/ container to an approved waste disposal plant.</p>
Human Complement C5b-9 Quality Control	HC5B9-6140		<p>Danger. Causes serious eye damage. Harmful if inhaled. May cause damage to organs Respiratory Tract through prolonged or repeated exposure. Harmful to aquatic life with long lasting effects. Do not breathe dust. Use only outdoors or in a well-ventilated area. Avoid release to the environment. Wear eye protection/ face protection. IF INHALED: Remove person to fresh air and keep comfortable for breathing. Call a POISON CENTER/ doctor if you feel unwell. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. Get medical advice/ attention if you feel unwell. Dispose of contents/ container to an approved waste disposal plant.</p>

Ingredient	Catalogue No.	Label	
Human Complement C5b-9 Detection	HC5B9-1140		<p>Warning. Causes serious eye irritation. May cause damage to organs Respiratory Tract through prolonged or repeated exposure .Do not breathe the mist or vapours. Wash skin thoroughly after handling. Wear eye protection/ face protection. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. Get medical advice/ attention if you feel unwell. If eye irritation persists: Get medical advice/ attention. Dispose of contents/ container to an approved waste disposal plant.</p>
Standard Matrix	MXHSM-C5B9		<p>Danger. Harmful if swallowed or if inhaled. Toxic in contact with skin. Causes serious eye damage. May cause damage to organs Respiratory Tract through prolonged or repeated exposure .May cause damage to organs Brain through prolonged or repeated exposure if swallowed. Harmful to aquatic life with long lasting effects. Do not breathe dust. Wash skin thoroughly after handling. Do not eat, drink or smoke when using this product. Use only outdoors or in a well-ventilated area. Avoid release to the environment. Wear protective gloves/ protective clothing/ eye protection/ face protection. IF SWALLOWED: Call a POISON CENTER/ doctor if you feel unwell. Rinse mouth. IF ON SKIN: Wash with plenty of water. Call a POISON CENTER/ doctor if you feel unwell. IF INHALED: Remove person to fresh air and keep comfortable for breathing. Call a POISON CENTER/ doctor if you feel unwell. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing. Get medical advice/ attention if you feel unwell. Take off contaminated clothing and wash before reuse. Store locked up. Dispose of contents/ container to an approved waste disposal plant.</p>

Ingredient	Catalogue No.	Label	
Assay Buffer	L-AB4		Warning. Causes serious eye irritation. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.
10X Wash Buffer	L-WB		Warning. May cause an allergic skin reaction. Wear protective gloves. IF ON SKIN: Wash with plenty of soap and water.
Streptavidin-Phycoerythrin	L-SAPE5		Warning: Causes serious eye irritation. IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

Technical Guidelines

To obtain reliable and reproducible results, the operator should carefully read this entire manual and fully understand all aspects of each assay step before running the assay. The following notes should be reviewed and understood before the assay is set up.

- FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.
- Do not use beyond the expiration date on the label.
- Do not mix or substitute reagents with those from other lots or sources.
- The Antibody-Immobilized Beads are light sensitive and must be protected from light at all times. Cover the assay plate containing beads with opaque plate lid or aluminum foil during all incubation steps.
- It is important to allow all reagents to warm to room temperature (20-25 °C) before use in the assay.
- Incomplete washing can adversely affect the assay outcome. All washing must be performed with the Wash Buffer provided.
- The standards prepared by serial dilution must be used within 1 hour of preparation.
Discard any unused standards except the standard stock which may be stored at ≤ -20 °C for 1 month and at ≤ -80 °C for greater than one month.
- If samples fall outside the dynamic range of the assay, further dilute the samples with the appropriate diluent and repeat the assay.
- Any unused mixed Antibody-Immobilized Beads may be stored in the Mixing Bottle at 2-8 °C for up to one month.
- During the preparation of the standard curve, make certain to mix the higher concentration well before making the next dilution. Use a new tip with each dilution.
- The plate should be read immediately after the assay is finished. If, however, the plate cannot be read immediately, seal the plate, cover with aluminum foil or an opaque lid, and store the plate at 2-8 °C for up to 24 hours. Prior to reading, agitate the plate on the plate shaker at room temperature for 10 minutes. Delay in reading a plate may result in decreased sensitivity for some analytes.
- The titer plate shaker should be set at a speed to provide maximum orbital mixing without splashing of liquid outside the wells. For the recommended plate shaker, this would be a setting of 5-7 which is approximately 500-800 rpm.
- Ensure that the needle probe is clean. This may be achieved by sonication and/or alcohol flushes.
- When reading the assay on Luminex[®] 200™, adjust probe height according to the protocols recommended by Luminex[®] to the kit solid plate or to the recommended filter plates using 3 alignment discs. When reading the assay on MAGPIX[®], adjust probe height according to the protocols recommended by Luminex[®] to the kit solid plate or to the recommended filter plates using 2 alignment discs. When reading the assay on FLEXMAP 3D[®], adjust probe height according to the protocols recommended by Luminex[®] to the kit solid plate using 1 alignment disc.
For FLEXMAP 3D[®] when using the solid plate in the kit, the final resuspension should be with 150 μ L Sheath Fluid PLUS in each well and 75 μ L should be aspirated.

For research use only. Not for use in diagnostic procedures.

For xMAP® INTELLIFLEX, adjust probe height based on the type of plate you are using, place an alignment disk or an alignment sphere in the well according to the protocol recommended by Luminex®.

- For cell culture supernatants or tissue extraction, use the culture or extraction medium as the matrix solution in background, standard curve, and control wells. If samples are diluted in Assay Buffer, use the Assay Buffer as matrix.
- For cell/tissue homogenate, the final cell or tissue homogenate should be prepared in a buffer that has a neutral pH, contains minimal detergents or strong denaturing detergents, and has an ionic strength close to physiological concentration. Avoid debris, lipids, and cell/tissue aggregates. Centrifuge samples before use.
- For serum/plasma samples that require further dilution beyond 1:100 (serum) or 1:20 (plasma) , use the Assay Buffer provided in the kit.
- Complement activation can occur in samples that are not handled properly. Proper sample collection, handling, and storage is necessary to achieve accurate assay results.
- Serum samples will typically produce higher complement values. EDTA Plasma is recommended to achieve the most accurate complement values.
- Vortex all reagents well before adding to plate.

Sample Collection and Storage

Preparation of Serum Samples

- Allow the blood to clot for at least 30 minutes before centrifugation for 10 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20 °C.
- Avoid multiple (> 2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- Serum samples should be diluted 1:100 in the Assay Buffer provided in the kit. For example, in a tube, 5 μ L of serum may be combined with 45 μ L of Assay Buffer (1:10), then add 10 μ L of 1:10 diluted serum to 90 μ L of Assay Buffer. When further dilution beyond 1:100 is required, use Assay Buffer as the diluent.

Preparation of Plasma Samples

- Plasma collection using EDTA as an anti-coagulant is recommended. Centrifuge for 10 minutes at 1000 x g within 30 minutes of blood collection. Remove plasma and assay immediately or aliquot and store samples at ≤ -20 °C.
- Avoid multiple (> 2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- Plasma samples should be diluted 1:20 in the Assay Buffer provided in the kit. For example, in a tube, 10 μ L of plasma may be combined with 190 μ L of Assay Buffer. When further dilution beyond 1:20 is required, use Assay Buffer as the diluent.

Preparation of Tissue Culture Supernatant

- Centrifuge the sample to remove debris and assay immediately or aliquot and store samples at ≤ -20 °C.
- Avoid multiple (> 2) freeze/thaw cycles.
- Tissue culture supernatant may require a dilution with an appropriate control medium prior to assay. Tissue/cell extracts should be done in neutral buffers containing reagents and conditions that do not interfere with assay performance. Excess concentrations of detergent, salt, denaturants, high or low pH, etc. will negatively affect the assay. Organic solvents should be avoided. The tissue/cell extract samples should be free of particles such as cells or tissue debris.

Note:

- A maximum of 25 μ L per well of 1:100 diluted serum or 1:20 diluted plasma can be used. Tissue culture or other media may also be used.
- All samples must be stored in polypropylene tubes. DO NOT STORE SAMPLES IN GLASS.
- Avoid debris, lipids and cells when using samples with gross hemolysis or lipemia.
- Care must be taken when using heparin as an anti-coagulant since an excess of heparin will provide falsely high values. Use no more than 10 IU heparin per mL of blood collected.

For research use only. Not for use in diagnostic procedures.

Preparation of Reagents for Immunoassay

Preparation of Antibody-Immobilized Beads

For **individual vials of beads**, sonicate each antibody-bead vial for 30 seconds; vortex for 1 minute. Add 150 μ L from each antibody-bead vial to the Mixing Bottle and bring final volume to 3.0 mL with bead diluent. Vortex the mixed beads well. Unused portion may be stored at 2-8 $^{\circ}$ C for up to one month.

Note: Due to the composition of magnetic beads, you may notice a slight color in the bead solution. This does not affect the performance of the beads or the kit.

Example: When using 1 antibody-immobilized beads, add 150 μ L from each of the 1 bead vials to the Mixing Bottle. Then add 2.85 mL bead diluent.

Preparation of Quality Controls

Before use, reconstitute Quality Control 1 and Quality Control 2 with 250 μ L deionized water. Invert the vial several times to mix and vortex. Allow the vial to sit for 5-10 minutes. Transfer the reconstituted Quality Control 1 and Quality Control 2 into two polypropylene microfuge tubes. Unused portion may be stored at \leq -20 $^{\circ}$ C for up to one month.

Preparation of Wash Buffer

Bring the 10X Wash Buffer to room temperature and mix to bring all salts into solution. Dilute 60 mL of 10X Wash Buffer with 540 mL deionized water. Store the unused portion at 2-8 $^{\circ}$ C for up to one month.

Preparation of Standard Matrix

This step is required for serum or plasma samples only.

Add 1.0 mL deionized water to the bottle containing lyophilized Standard Matrix. Mix well. Allow at least 10 minutes for complete reconstitution. Leftover reconstituted Standard Matrix should be stored at \leq -20 $^{\circ}$ C for up to one month.

Preparation of Human Complement C5b-9 Standard


1. Prior to use, reconstitute the Human Complement C5b-9 Standard with 250 μL deionized water. Refer to table below for analyte concentrations. Invert the vial several times to mix. Vortex the vial for 10 seconds. Allow the vial to sit for 5-10 minutes. Transfer the reconstituted standard to a polypropylene microfuge tube. This will be used as the 450 ng/mL Standard; the unused portion may be stored at $\leq -20\text{ }^{\circ}\text{C}$ for up to one month.
2. Preparation of Working Standards

Label 6 polypropylene microfuge tubes Standard 1 through Standard 6. Add 200 μL of Assay Buffer to each of the 6 tubes. Prepare serial dilutions by adding 100 μL of the reconstituted standard to the Standard 6 tube, mix well and transfer 100 μL of Standard 6 to the Standard 5 tube, mix well and transfer 100 μL of Standard 5 to the Standard 4 tube, mix well and transfer 100 μL of Standard 4 to the Standard 3 tube, mix well and transfer 100 μL of Standard 3 to the Standard 2 tube, mix well and transfer 100 μL of Standard 2 to the Standard 1 tube and mix well. The 0 ng/mL standard (Background) will be Assay Buffer.

Standard Concentration (ng/mL)	Volume of Deionized Water to Add	Volume of Standard to Add
450 ng/mL	250 μL	0

Standard Concentration (ng/mL)	Volume of Assay Buffer to Add	Volume of Standard to Add
150 ng/mL	200 μL	100 μL of 450 ng/mL
50 ng/mL	200 μL	100 μL of 150 ng/mL
16 ng/mL	200 μL	100 μL of 50 ng/mL
5.6 ng/mL	200 μL	100 μL of 16 ng/mL
1.9 ng/mL	200 μL	100 μL of 5.6 ng/mL
0.6 ng/mL	200 μL	100 μL of 1.9 ng/mL

Preparation of Standards

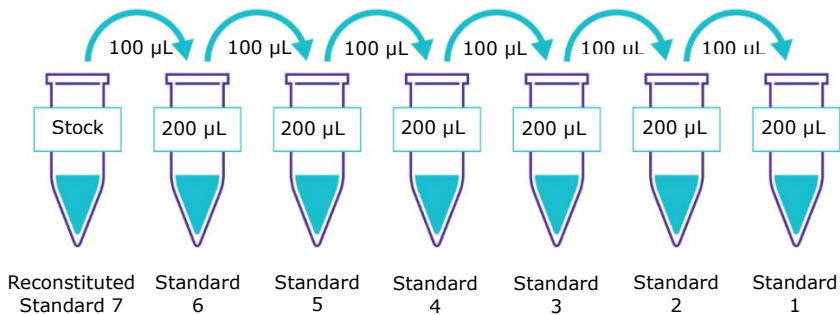

Immunoassay Procedure

- Prior to beginning this assay, it is imperative to read this protocol completely and to thoroughly understand the Technical Guidelines.
- Allow all reagents to warm to room temperature (20-25 °C) before use in the assay.
- Diagram the placement of Standards 0 (Background), 0.6 ng/mL through 450 ng/mL standards, Controls 1 and 2, and Samples on Well Map Worksheet in a vertical configuration. It is recommended to run the assay in duplicate.

Note: Most instruments will only read the 96-well plate vertically by default.

- If using a filter plate, set the filter plate on a plate holder at all times during reagent dispensing and incubation steps so that the bottom of the plate does not touch any surface.

3. Add 200 μ L of Wash buffer into each well of the plate. Seal and mix on a plate shaker for 10 minutes at room temperature (20-25 °C).
4. Decant wash buffer and remove the residual amount from all wells by inverting the plate and tapping it smartly onto absorbent towels several times.
5. Add 25 μ L of each Standard or Control into the appropriate wells. Assay Buffer should be used for 0 standard (Background).
6. Add 25 μ L of Assay Buffer to the sample wells.
7. Add 25 μ L of appropriate matrix solution to the background, standards, and control wells. When assaying serum or plasma, use the Standard Matrix. When assaying tissue culture or other supernatant, use proper control culture medium as the matrix solution.
8. Add 25 μ L of Sample (diluted) into the appropriate wells.
9. Vortex Mixing Bottle and add 25 μ L of the Mixed Beads to each well.
10. **Note:** During addition of Beads, shake bead bottle intermittently to avoid settling.
11. Seal the plate with a plate sealer. Wrap the plate with foil and incubate with agitation on a plate shaker overnight (16-18 hours) at 2-8 °C. Alternatively, incubate for 2 hours at room temperature (20-25 °C).

Add 200 μ L Wash Buffer per well



Shake 10 min, RT
Decant

- Add 25 μ L Standard or Control to appropriate wells
- Add 25 μ L Assay Buffer to background and sample wells
- Add 25 μ L appropriate matrix solution to background, standards, and control wells
- Add 25 μ L diluted Samples to sample wells
- Add 25 μ L Beads to each well



Incubate overnight (16-18 hours) at 2-8 °C or 2 hours at room temperature (20-25 °C)

- Gently remove well contents and wash plate 3 times following instructions listed in the **PLATE WASHING** section.

- Add 25 μL of Detection Antibodies into each well.

Note: Allow the Detection Antibodies to warm to room temperature prior to addition.

- Seal, cover with foil and incubate with agitation on a plate shaker for 1 hour at room temperature (20-25 $^{\circ}\text{C}$).
- Gently remove well contents and wash plate 3 times following instructions listed in the **PLATE WASHING** section.
- Add 25 μL Streptavidin-Phycoerythrin to each well.
- Seal, cover with foil and incubate with agitation on a plate shaker for 30 minutes at room temperature (20-25 $^{\circ}\text{C}$).

- Gently remove well contents and wash plate 3 times following instructions listed in the **PLATE WASHING** section.

- Add 150 μL of Sheath Fluid PLUS (or Drive Fluid PLUS if using MAGPIX[®]) to all wells. Resuspend the beads on a plate shaker for 5 minutes.

- Run plate on Luminex[®] 200[™], HTS, FLEXMAP 3D[®], MAGPIX[®] with xPONENT[®] software or xMAP[®] INTELLIFLEX with INTELLIFLEX Software.

- Save and analyze the Median Fluorescent Intensity (MFI) data using a 5-parameter logistic or spline curve-fitting method for calculating analyte concentrations in samples.

Note: For diluted samples, final sample concentrations should be multiplied by the dilution factor. For samples diluted as per protocol instructions, multiply by 100 (serum) or 20 (plasma). If using another dilution factor, multiply by the appropriate dilution factor.



Remove well contents and wash 3X with 200 μL Wash Buffer

Add 25 μL Detection Antibodies per well



Incubate 1 hour at RT

Remove well contents and wash 3X with 200 μL Wash Buffer

Add 25 μL Streptavidin-Phycoerythrin per well



Incubate 30 minutes at RT

Remove well contents and wash 3X with 200 μL Wash Buffer

Add 150 μL Sheath Fluid PLUS or Drive Fluid PLUS per well

Read on Luminex[®] instrument (100 μL , 50 beads per bead set)

Plate Washing

If using a solid plate, use either a handheld magnet or magnetic plate washer.

Solid Plate

- Handheld magnet (Catalogue No. 40-285)

Rest plate on magnet for 60 seconds to allow complete settling of magnetic beads. Remove well contents by gently decanting the plate in an appropriate waste receptacle and gently tapping on absorbent pads to remove residual liquid. Wash plate with 200 μ L of Wash Buffer by removing plate from magnet, adding Wash Buffer, shaking for 30 seconds, reattaching to magnet, letting beads settle for 60 seconds and removing well contents as previously described after each wash. Repeat wash steps as recommended in Assay Procedure.
- Magnetic plate washer (Catalogue Nos. 40-094, 40-095, 40-096 and 40-097)

Please refer to specific automatic plate washer manual for appropriate equipment settings. Please note that after the final aspiration, there will be approximately 25 μ L of residual wash buffer in each well. This is expected when using the BioTek® plate washer and this volume does not need to be aspirated from the plate.

If using an automatic plate washer other than BioTek® 405 LS or 405 TS, please refer to the manufacturer's recommendations for programming instructions.

Filter Plate

(Catalogue No. MX-PLATE)

If using a filter plate, use a vacuum filtration manifold to remove well contents. Wash plate with 200 μ L/well of Wash Buffer, removing Wash Buffer by vacuum filtration after each wash. Repeat wash steps as recommended in the Assay Procedure.

Equipment Settings

Luminex® 200™, HTS, FLEXMAP 3D®, MAGPIX® with xPONENT® software and xMAP® INTELLIFLEX with INTELLIFLEX software:

These specifications are for the above listed instruments and software. Luminex® instruments with other software (for example MasterPlex®, StarStation, LiquiChip, Bio-Plex® Manager™, LABScan™100) would need to follow instrument instructions for gate settings and additional specifications from the vendors for reading Luminex® magnetic beads.

For magnetic bead assays, each instrument must be calibrated, and performance verified with the indicated calibration and verification kits.

Instrument	Calibration Kit	Verification Kit
Luminex® 200™ and HTS	xPONENT® 3.1 compatible Calibration Kit (Catalogue No. LX2R-CAL-K25)	Performance Verification Kit (Catalogue No. LX2R-PVER-K25)
FLEXMAP 3D®	FLEXMAP 3D® Calibrator Kit (Catalogue No. F3D-CAL-K25)	FLEXMAP 3D® Performance Verification Kit (Catalogue No. F3D-PVER-K25)
xMAP® INTELLIFLEX	xMAP® INTELLIFLEX Calibration Kit (Catalogue No. IFX-CAL-K20)	xMAP® INTELLIFLEX Performance Verification Kit (Catalogue No. IFX-PVER-K20)
MAGPIX®	MAGPIX® Calibration Kit (Catalogue No. MPX-CAL-K25)	MAGPIX® Performance Verification Kit (Catalogue No. MPX-PVER-K25)

Note: When setting up a Protocol using the xPONENT® software, you must select MagPlex® as the Bead Type in the Acquisition settings.

Note: These assays cannot be run on any instruments using Luminex® IS 2.3 or Luminex® 1.7 software.

The Luminex® probe height must be adjusted to the plate provided in the kit. Please use Catalogue No. MAG-PLATE, if additional plates are required for this purpose.

Events	50, per bead
Sample Size	100 µL
Gate Settings	8,000 to 15,000
Reporter Gain	Default (low PMT)
Time Out	60 seconds
Bead Set	Customizable 1-plex Beads
	C5b-9
	56

Quality Controls

The ranges for each analyte in Quality Control 1 and 2 are provided on the card insert or can be located at our website SigmaAldrich.com using the catalogue number as the keyword.

Assay Characteristics

Cross-Reactivity

Cross-Reactivity between C5b-9 and other complement proteins found in MILLIPLEX® Human Complement Expanded panel 1 (Cat. No. HCMPEX1-19K) and MILLIPLEX® Human Complement Panel 2 (Cat. No. HCMP2MAG-19K) was tested. There was no or negligible cross-reactivity between the antibody pair in this panel for any of the analytes tested.

Assay Sensitivities

(minimum detectable concentrations, ng/mL)

Minimum Detectable Concentration (MinDC) is calculated using MILLIPLEX® Analyst 5.1. It measures the true limits of detection for an assay by mathematically determining what the empirical MinDC would be if an infinite number of standard concentrations were run for the assay under the same conditions.

Analyte	Overnight Protocol (n = 9 Assays)		2-Hour Protocol (n = 3 Assays)	
	MinDC (ng/mL)	MinDC+2SD (ng/mL)	MinDC (ng/mL)	MinDC+2SD (ng/mL)
C5b-9	0.08	0.16	0.08	0.21

Precision

Intra-assay precision is generated from the mean of the %CVs from 8 reportable results across two different concentrations of analytes in a single assay. Inter-assay precision is generated from the mean of the % CVs across two different concentrations of analytes across 5 different assays.

Analyte	Overnight Protocol		2-Hour Protocol
	Intra-assay %CV	Inter-assay %CV	Intra-assay %CV
C5b-9	< 15%	< 15%	< 10%

Accuracy

Spike Recovery: The data represent mean percent recovery of spiked standards ranging from low, medium, and high concentration in serum and plasma samples (n=10).

Analyte	Overnight Protocol	2-Hour Protocol
	% Recovery in Sample	% Recovery in Sample
C5b-9	120%	100%

Troubleshooting

Problem	Probable Cause	Solution
	Plate washer aspirate height set too low	Adjust aspiration height according to manufacturers' instructions.
	Bead mix prepared inappropriately	Sonicate bead vials and vortex just prior to adding to bead mix bottle according to protocol. Agitate bead mix intermittently in reservoir while pipetting this into the plate.
	Samples cause interference due to particulate matter or viscosity	See above. Also sample probe may need to be cleaned with alcohol flushes, back flushes, and washes; or, if needed, probe should be removed and sonicated.
Insufficient bead count	Probe height not adjusted correctly	<p>When reading the assay on Luminex® 200™, adjust probe height to the kit solid plate or to the recommended filter plates using 3 alignment discs. When reading the assay on MAGPIX®, adjust probe height to the kit solid plate or to the recommended filter plates using 2 alignment discs. When reading the assay on FLEXMAP 3D®, adjust probe height to the kit solid plate using 1 alignment disc. For FLEXMAP 3D® when using the solid plate in the kit, the final resuspension should be with 150 µL Sheath Fluid PLUS in each well and 75 µL should be aspirated.</p> <p>When reading the assay on xMAP® INTELLIFLEX, adjust probe height based on the type of plate you are using, place an alignment disk or an alignment sphere in the well according to the protocol recommended by Luminex®.</p>

Problem	Probable Cause	Solution
Background is too high	Background wells were contaminated	Avoid cross-well contamination by using sealer appropriately and pipetting with multichannel pipettes without touching reagent in plate.
	Matrix used has endogenous analyte or interference	Check matrix ingredients for cross-reacting components (for example, interleukin modified tissue culture medium).
	Insufficient washes	Increase number of washes.
Beads not in region or gate	Luminex® instrument not calibrated correctly or recently	Calibrate Luminex® instrument based on manufacturer's instructions, at least once a week or if temperature has changed by >3 °C.
	Gate settings not adjusted correctly	Some Luminex® instruments (for example Bio-Plex®) require different gate settings than those described in the kit protocol. Use instrument default settings.
	Wrong bead regions in protocol template	Check kit protocol for correct bead regions or analyte selection.
	Incorrect sample type used	Samples containing organic solvents or if highly viscous should be diluted or dialyzed as required.
	Instrument not washed or primed	Prime the Luminex® instrument 4 times to rid it of air bubbles, wash 4 times with Sheath Fluid PLUS or water if there is any remnant alcohol or sanitizing liquid.
	Beads were exposed to light	Keep plate and bead mix covered with dark lid or aluminum foil during all incubation steps.

Problem	Probable Cause	Solution
Signal for whole plate is same as background	Incorrect or no Detection Antibody was added	Add appropriate Detection Antibody and continue.
	Streptavidin-Phycoerythrin was not added	Add Streptavidin-Phycoerythrin according to protocol. If Detection Antibody has already been removed, sensitivity may be low.
Low signal for standard curve	Detection Antibody may have been removed prior to adding Streptavidin-Phycoerythrin	May need to repeat assay if desired sensitivity not achieved.
	Incubations done at inappropriate temperatures, timings, or agitation	Assay conditions need to be checked.
Signals too high, standard curves are saturated	Calibration target value set too high	With some Luminex [®] instruments (for example, Bio-Plex [®]) default target setting for RP1 calibrator is set at high PMT. Use low target value for calibration and reanalyze plate.
	Plate incubation was too long with standard curve and samples	Use shorter incubation time.
Sample readings are out of range	Samples contain no or below detectable levels of analyte	If below detectable levels, it may be possible to use higher sample volume. Check with technical support for appropriate protocol modifications.
	Samples contain analyte concentrations higher than highest standard point	Samples may require dilution and reanalysis for just that particular analyte.
	Standard curve was saturated at higher end of curve	See above.

For research use only. Not for use in diagnostic procedures.

Problem	Probable Cause	Solution
High variation in samples and/or standards	Multichannel pipette may not be calibrated	Calibrate pipettes.
	Plate washing was not uniform	Confirm all reagents are removed completely in all wash steps.
	Samples may have high particulate matter or other interfering substances	See above.
	Plate agitation was insufficient	Plate should be agitated during all incubation steps using an orbital plate shaker at a speed where beads are in constant motion without causing splashing.
	Cross-well contamination	Check when reusing plate sealer that no reagent has touched sealer. Care should be taken when using same pipette tips that are used for reagent additions and that pipette tip does not touch reagent in plate.

For Filter Plates Only

Filter plate will not vacuum	Vacuum pressure is insufficient	Increase vacuum pressure such that 0.2 mL buffer can be suctioned in 3-5 seconds.
	Samples have insoluble particles	Centrifuge samples just prior to assay set-up and use supernatant.
	High lipid concentration	After centrifugation, remove lipid layer and use supernatant.

Problem	Probable Cause	Solution
	Vacuum pressure too high	Adjust vacuum pressure such that 0.2 mL buffer can be suctioned in 3-5 seconds. May need to transfer contents to a new (blocked) plate and continue.
	Plate set directly on table or absorbent towels during incubations or reagent additions	Set plate on plate holder or raised edge so bottom of filter is not touching any surface.
Plate leaked	Insufficient blotting of filter plate bottom causing wicking	Blot the bottom of the filter plate well with absorbent towels after each wash step.
	Pipette touching plate filter during additions	Pipette to the side of plate.
	Probe height not adjusted correctly	Adjust probe to 3 alignment discs in well H6.
	Sample too viscous	May need to dilute sample.

Product Ordering

Order products online at [SigmaAldrich.com](https://www.sigmaaldrich.com).

Replacement Reagents	Catalogue Number
Human Complement C5b-9 Standard	HC5B9-8140
Human Complement C5b-9 Quality Control	HC5B9-6140
Bead Diluent	LBD
Standard Matrix	MXHSM-C5B9
Human Complement C5b-9 Detection	HC5B9-1140
Streptavidin-Phycoerythrin	L-SAPE5
Assay Buffer	L-AB4
Set of two 96-Well plates with sealers	MAG-PLATE
10X Wash Buffer	L-WB

Antibody-Immobilized Magnetic Beads

Bead/Analyte Name	Bead No.	Catalogue Number
Anti-Human Complement C5b-9 bead	56	HC5B9-MAG

Well Map

	1	2	3	4	5	6	7	8	9	10	11	12
A	0 Standard ng/mL (Background)	16 ng/mL Standard	QC-1 Control	Etc.								
B	0 Standard ng/mL (Background)	16 ng/mL Standard	QC-1 Control									
C	0.6 ng/mL Standard	50 ng/mL Standard	QC-2 Control									
D	0.6 ng/mL Standard	50 ng/mL Standard	QC-2 Control									
E	1.9 ng/mL Standard	150 ng/mL Standard	Sample 1									
F	1.9 ng/mL Standard	150 ng/mL Standard	Sample 1									
G	5.6 ng/mL Standard	450 ng/mL Standard	Sample 2									
H	5.6 ng/mL Standard	450 ng/mL Standard	Sample 2									

For research use only. Not for use in diagnostic procedures.

Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

Technical Assistance

Visit the tech service page at SigmaAldrich.com/techservice.

Standard Warranty

The applicable warranty for the products listed in this publication may be found at SigmaAldrich.com/terms.

Contact Information

For the location of the office nearest you, go to SigmaAldrich.com/offices.

Safety Data Sheets (SDS)

Safety Data Sheets are available on the product page at SigmaAldrich.com.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

Merck, Millipore, Milliplex and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.

© 2023 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

For research use only. Not for use in diagnostic procedures.

